


-15kV TOF: -9051 v  
 -3.6kV MCP: -2688 v  
 -2.4kV MCP: -1589 v  
 Input Cur: 304 ma  
 RPA max: 236 v  
 Mirror max: 238 v

Tue Sep 26 12:14:00 2006

## TIDE Direct Events

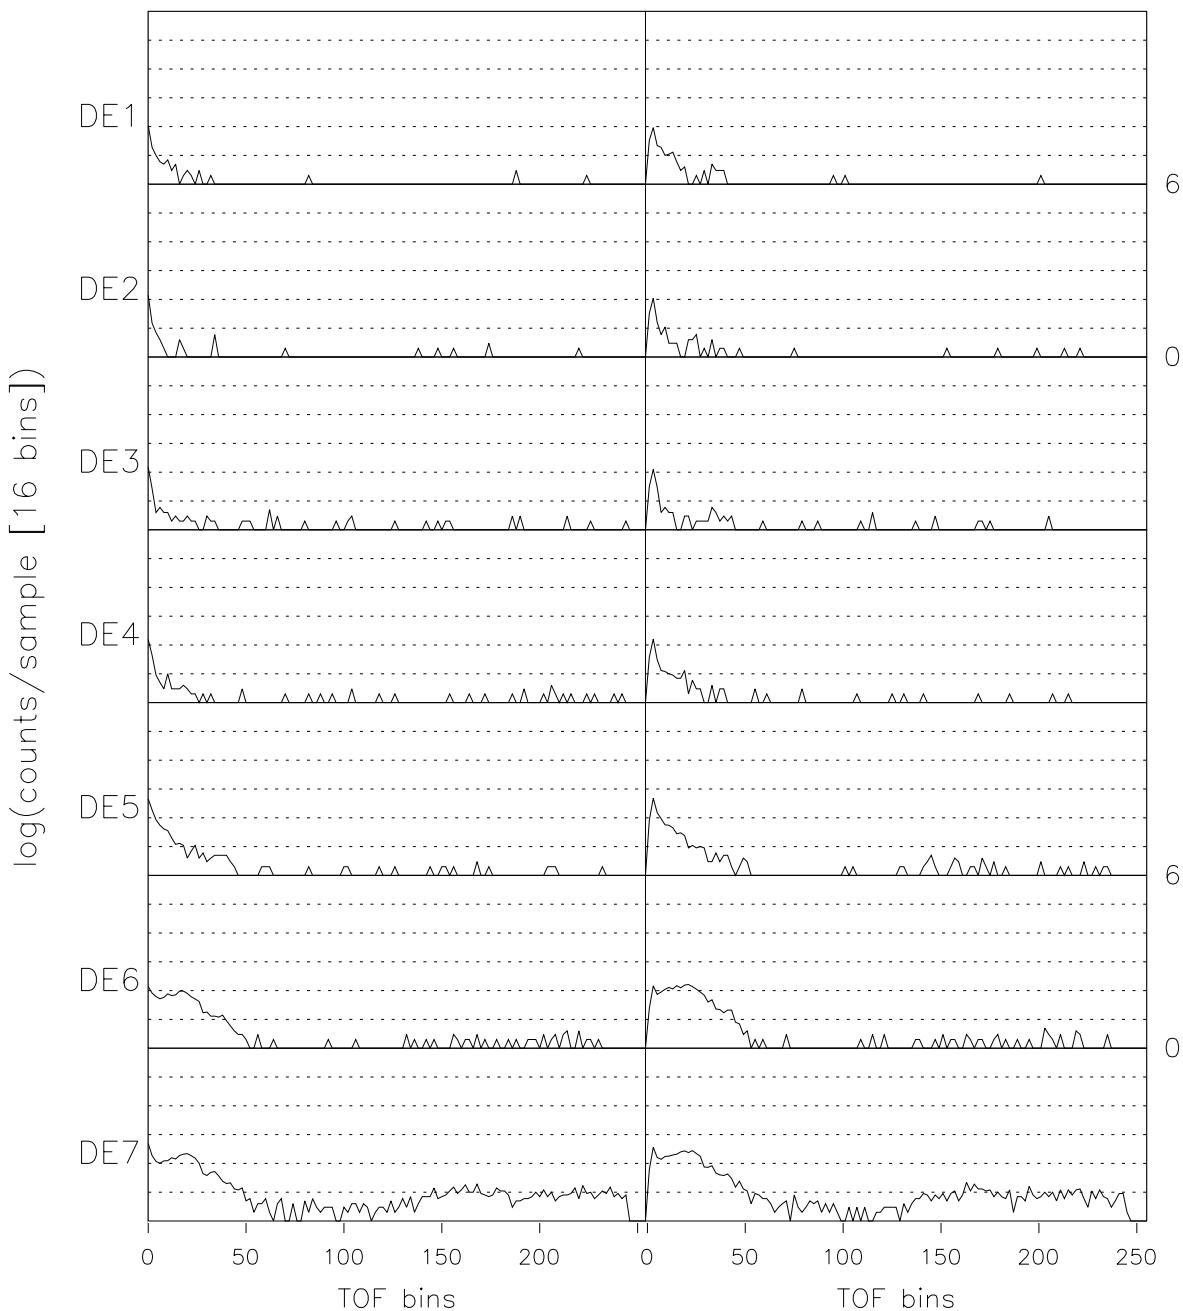

reported: 08-23-96 19:32:28 UT

reported: 08-23-96 19:35:39 UT

file: /export/data/tide/nrt/96082301.dat

-15kV TOF: -9181 v

-3.6kV MCP: -2672 v

-2.4kV MCP: -1579 v

Input Cur: 294 ma

RPA max: 236 v

Mirror max: 238 v